



S4 Fig. Sensitivity analysis of the system


Activation value (0.1): Modified activation rule with sigmoid transformation function

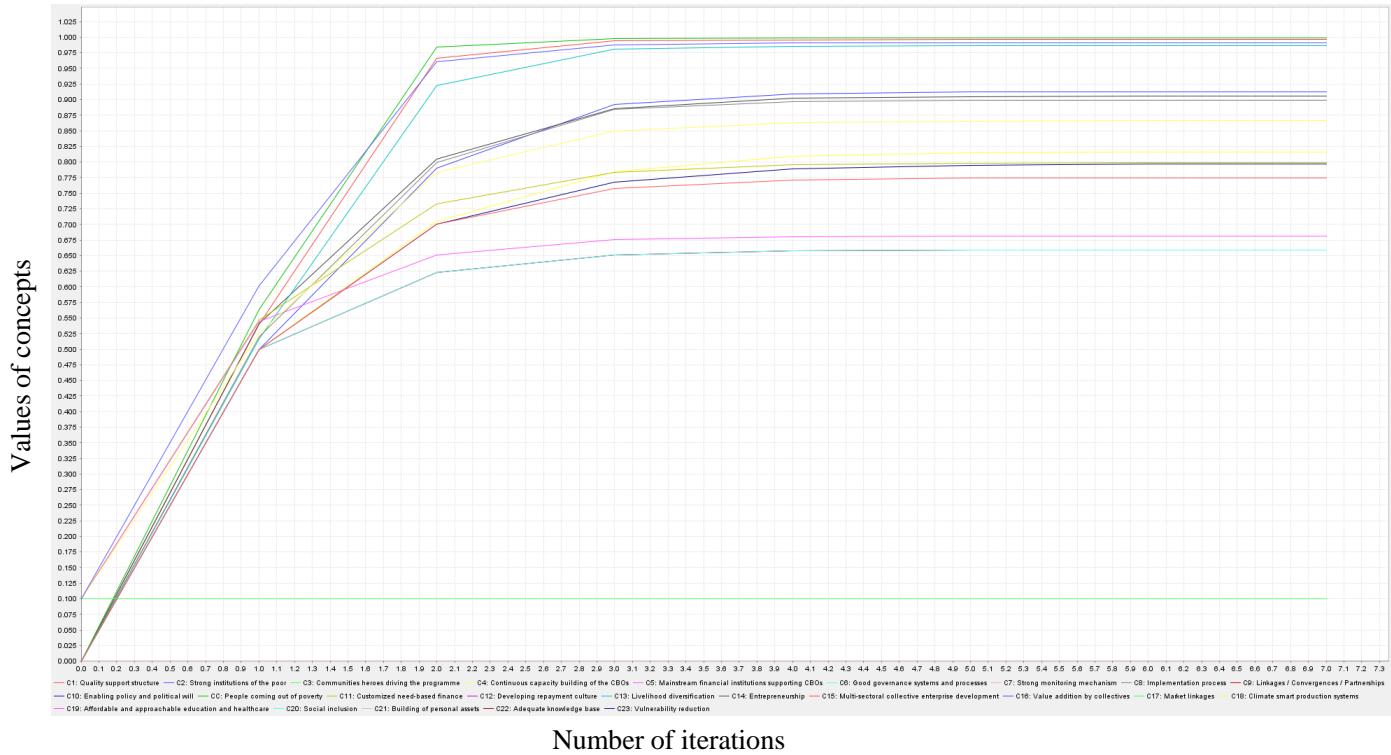


Activation value (0.2): Modified activation rule with sigmoid transformation function

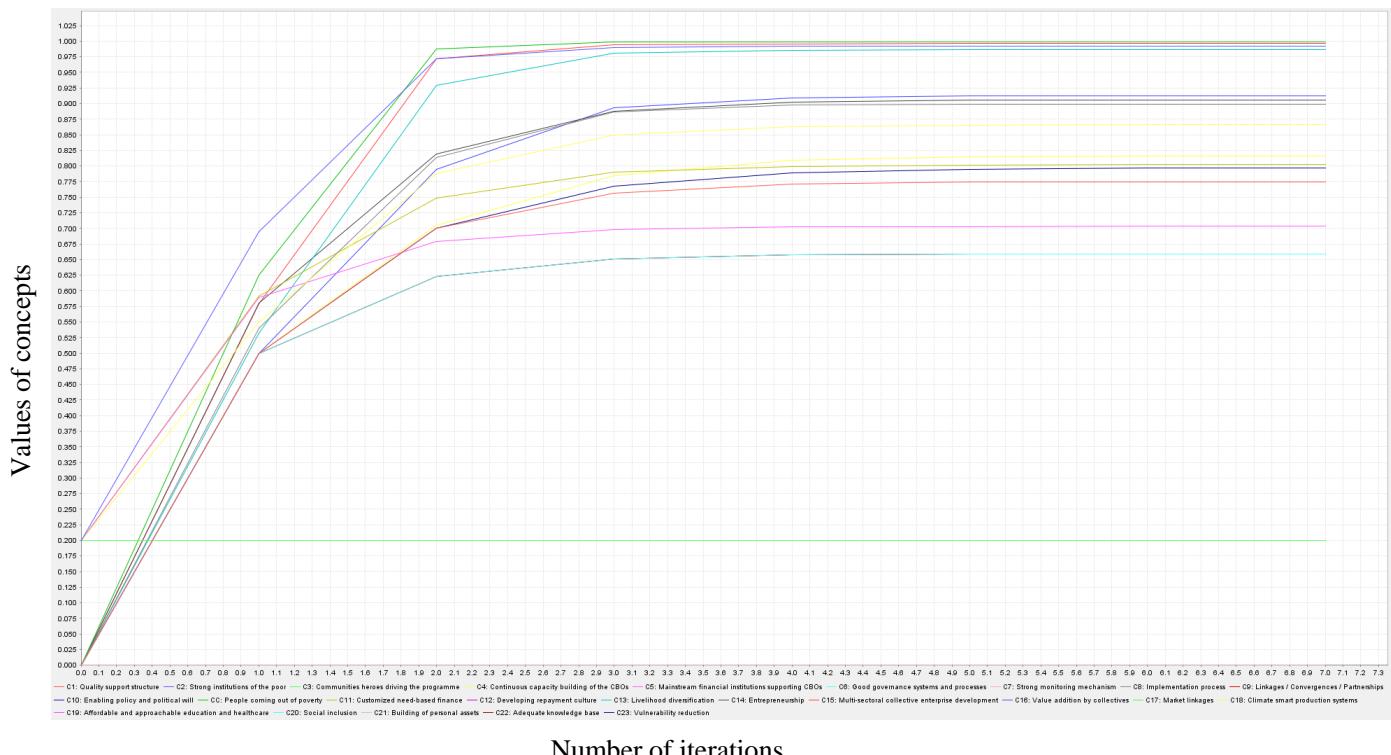

Activation value (0.3): Modified activation rule with sigmoid transformation function

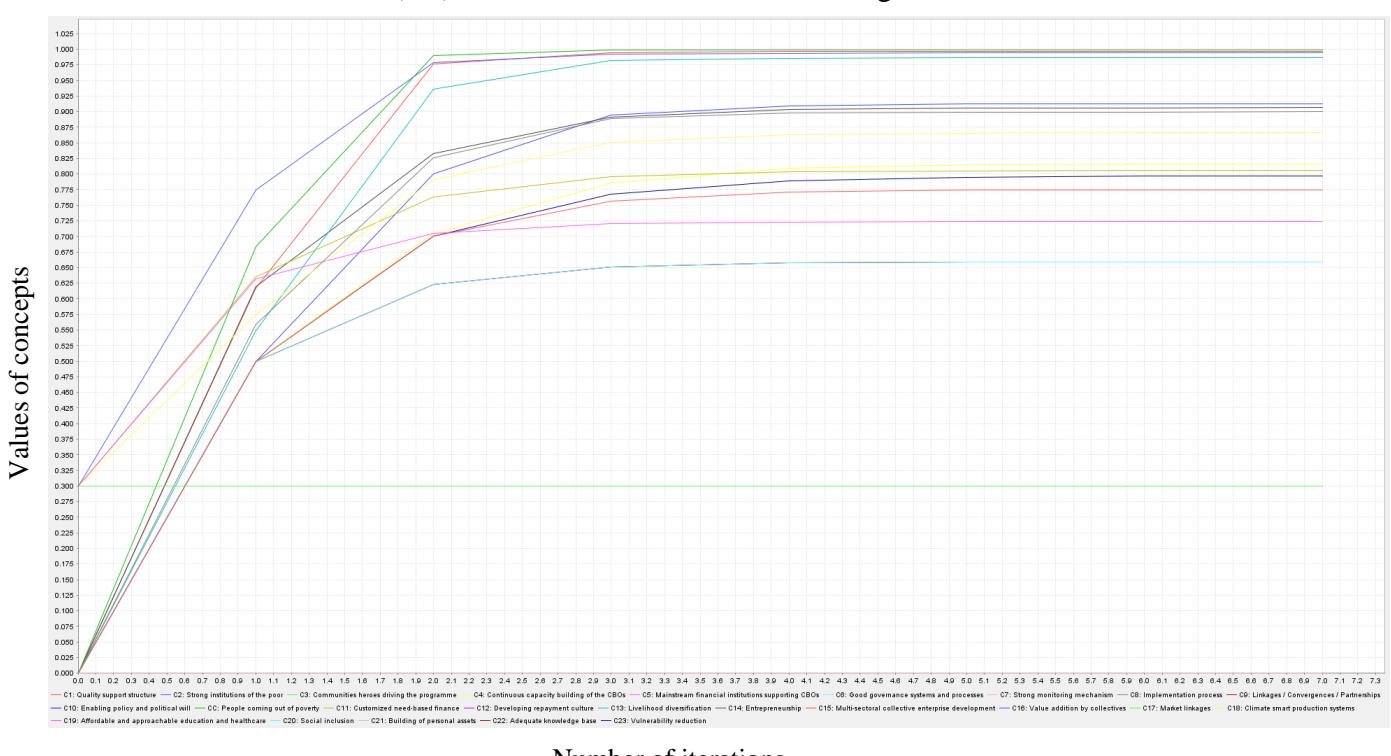


Activation value (0.4): Modified activation rule with sigmoid transformation function

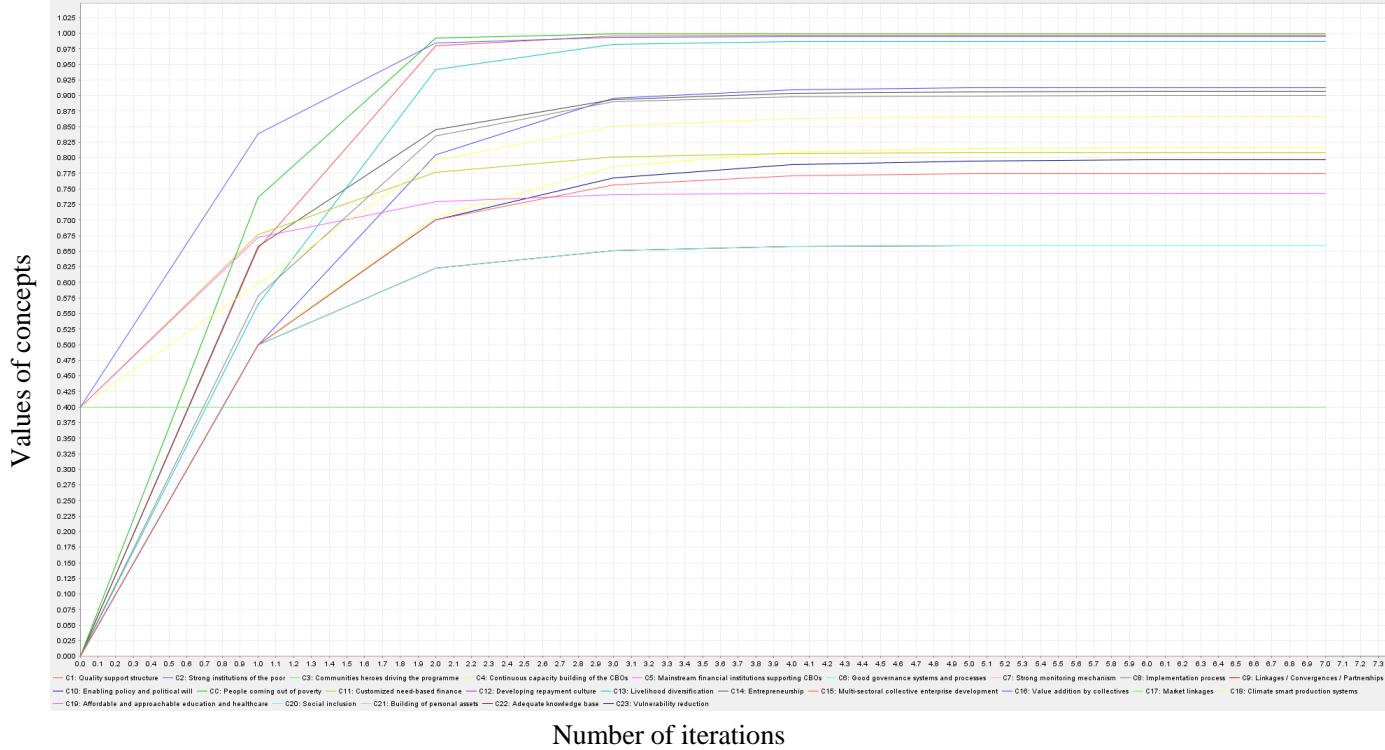


Number of iterations

Activation value (0.5): Modified activation rule with sigmoid transformation function

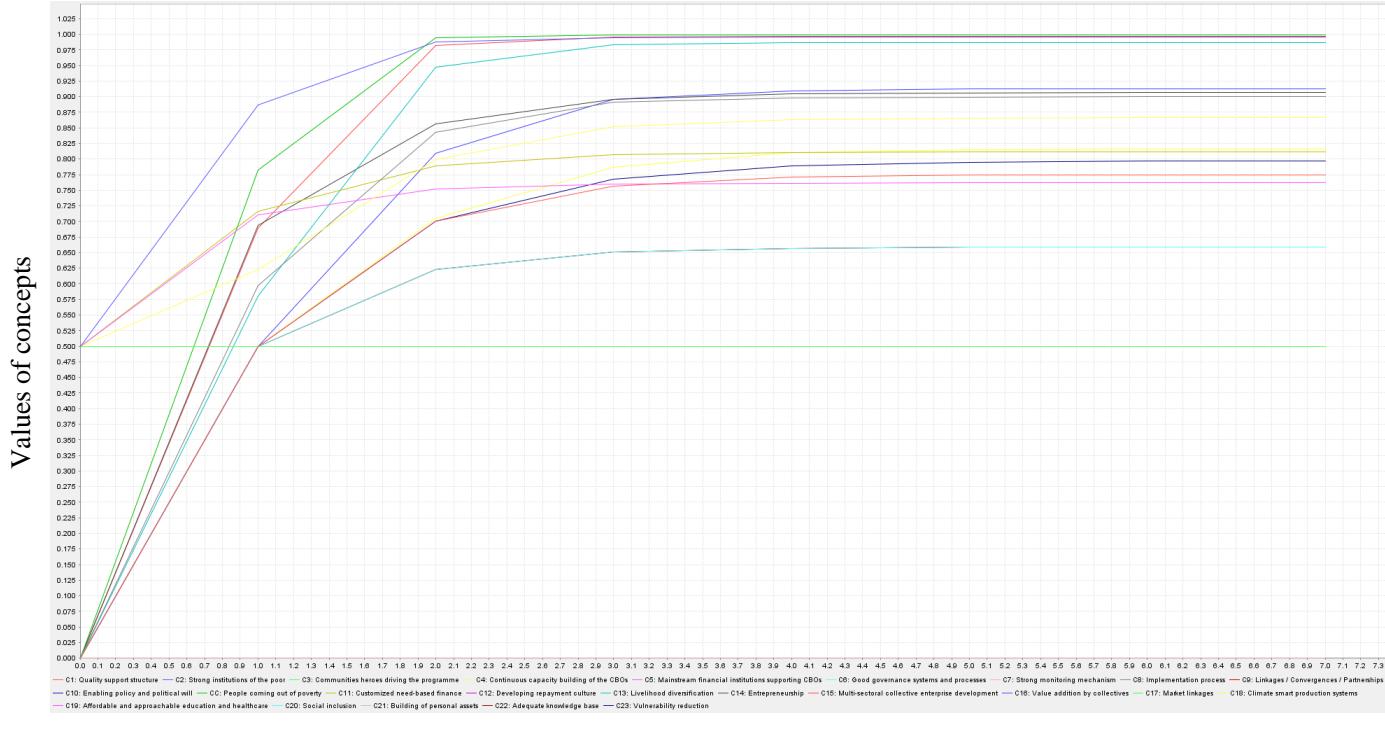


Number of iterations

Activation value (0.6): Modified activation rule with sigmoid transformation function

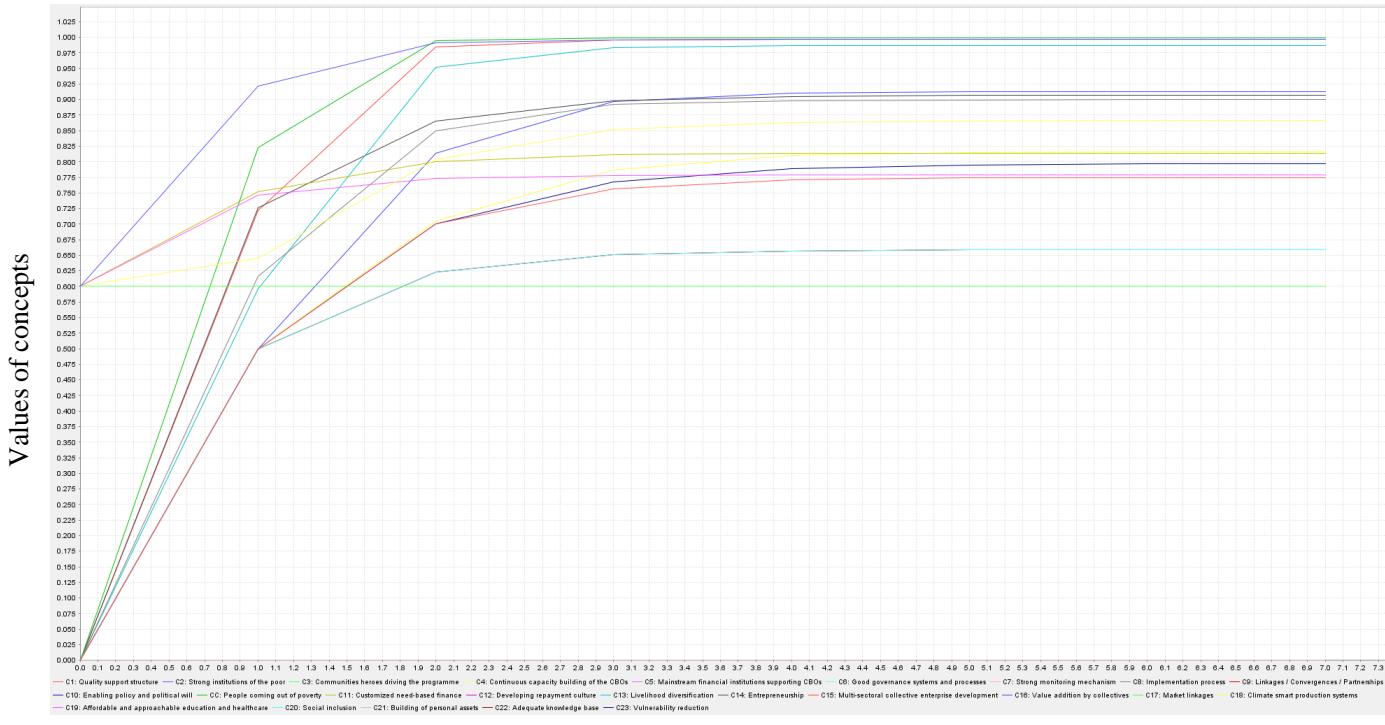


Number of iterations

Activation value (0.7): Modified activation rule with sigmoid transformation function

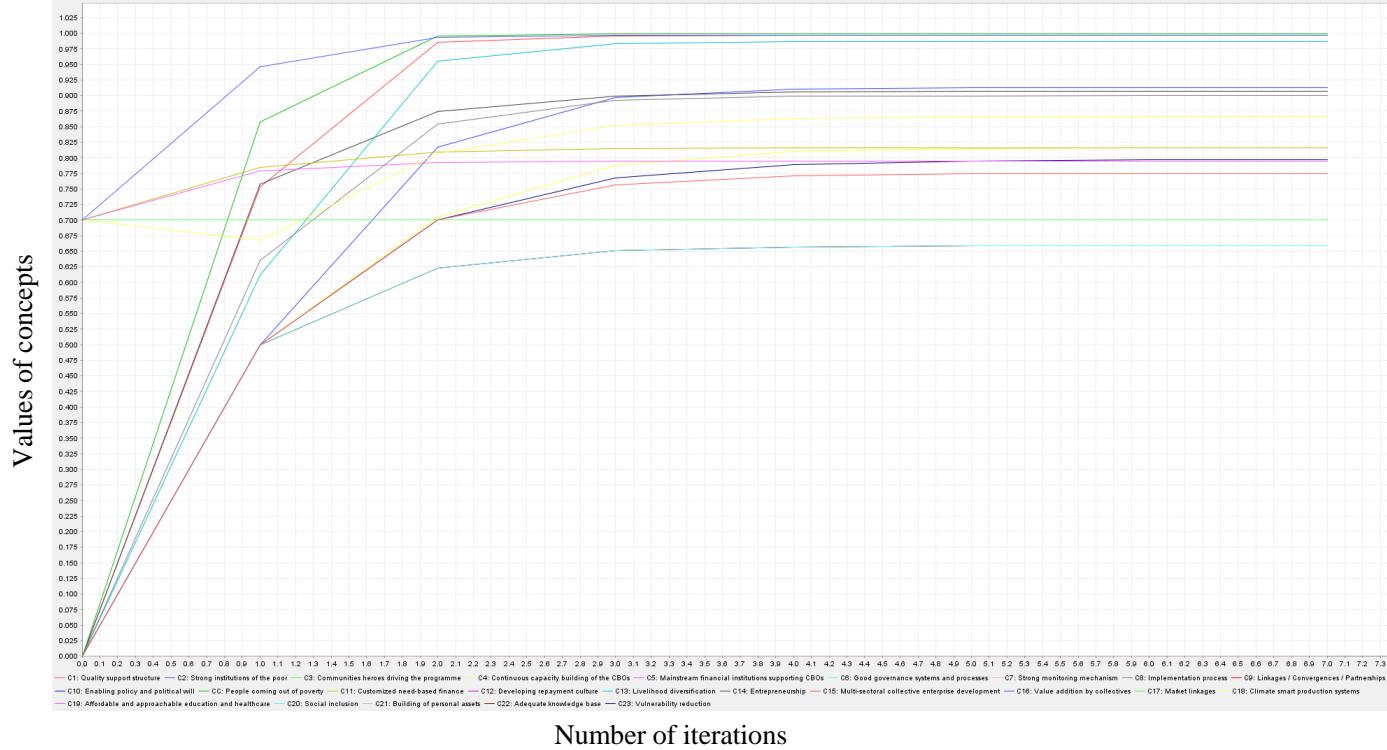

Activation value (0.8): Modified activation rule with sigmoid transformation function

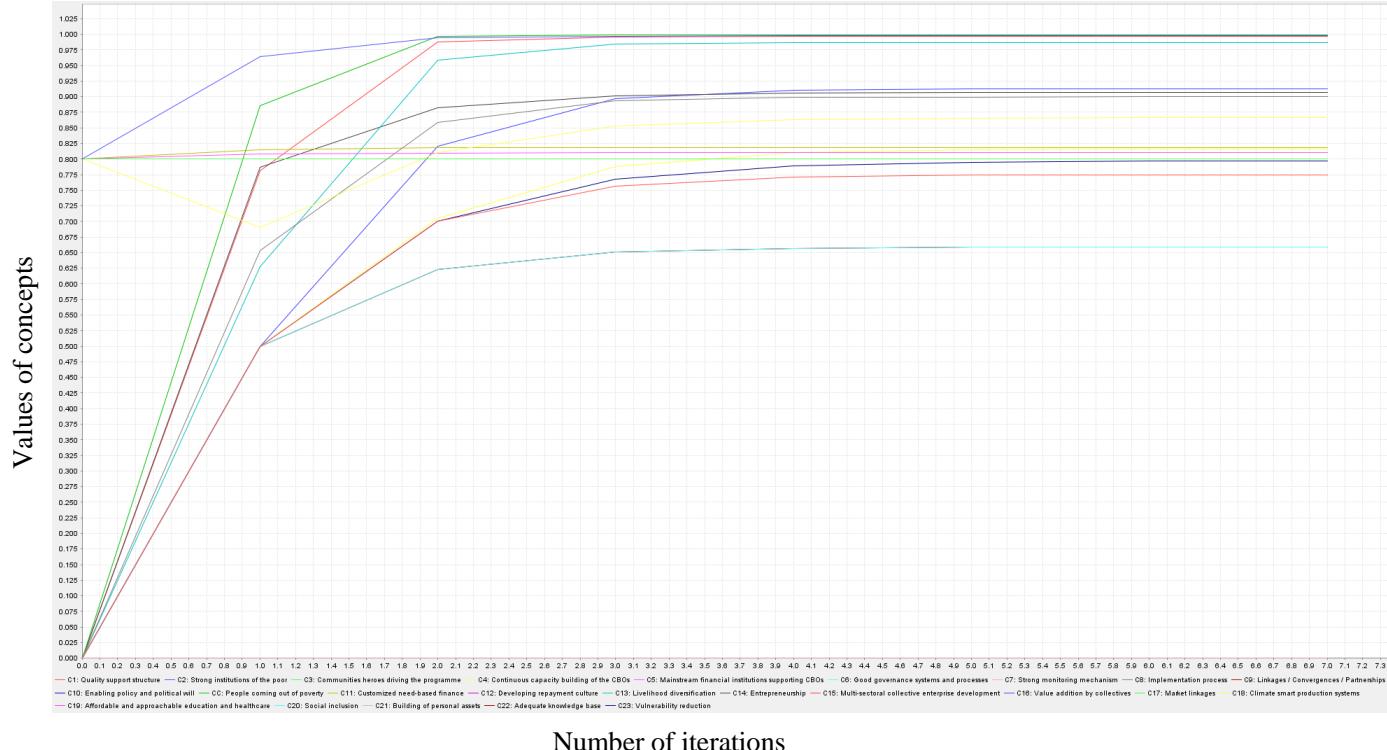

Activation value (0.9): Modified activation rule with sigmoid transformation function

